

# An Image Processing Approach to Pre-compensation for Higher-Order Aberrations in the Eye

Miguel Alonso Jr.

Department of Electrical and Computer Engineering, Florida International University  
Miami, FL, 33174, USA

and

Armando Barreto

Departments of Electrical and Computer Engineering and Biomedical Engineering,  
Florida International University, Miami, FL, 33174, USA

## ABSTRACT

Human beings rely heavily on vision for almost all of the tasks that are required in daily life. Because of this dependence on vision, humans with visual limitations, caused by genetic inheritance, disease, or age, will have difficulty in completing many of the tasks required of them. Some individuals with severe visual impairments, known as high-order aberrations, may have difficulty in interacting with computers, even when using a traditional means of visual correction (e.g., spectacles, contact lenses). This is, in part, because these correction mechanisms can only compensate for the most regular (low-order) distortions or aberrations of the image in the eye. This paper presents an image processing approach that will pre-compensate the images displayed on the computer screen, so as to counter the effect of the eye's aberrations on the image. The characterization of the eye required to perform this customized pre-compensation is the eye's Point Spread Function (PSF). Ophthalmic instruments generically called "Wavefront Analyzers" can now measure this description of the eye's optical properties. The characterization provided by these instruments also includes the "higher-order aberration components" and could, therefore, lead to a more comprehensive vision correction than traditional mechanisms. This paper explains the theoretical foundation of the methods proposed and illustrates them with experiments involving the emulation of a known and constant PSF by interposing a lens in the field of view of normally sighted test subjects.

**Keywords:** Point spread function, Optical transfer function, Retina, Deconvolution, Pre-deblurring, Deblurring

## 1. INTRODUCTION

Vision provides humans with a large proportion of the information they are able to gather from their surrounding environment. The sense of vision in humans has evolved into a highly refined system, allowing humans to see in three dimensions with high resolution and color [1]. The sense of sight is so important that, when limited by age or disease, it reduces a person's ability to perform otherwise ordinary tasks, such as interacting with a computer system.

Human beings perceive objects in their surroundings as images formed on their retinas inside their eyes [2]. However, the natural visual system of some individuals does not accurately map images from the outside world onto their retinas. The most common of these visual impairments include myopia, hyperopia, and astigmatism. All of them result in a retinal

representation of a point of light that is not confined to a single point on the retina. The distortion in the mapping of external images onto the retina is represented by the eye's "wavefront aberration function." Myopia, hyperopia, and astigmatism are referred to as low-order aberrations because the distortion they introduce can be modeled by first or second order Zernike polynomials. These "low-order" aberrations are currently corrected through spectacles or contact lenses, which modify the external images before they reach the eye.

In some cases, however, a low-order Zernike model is not sufficient to completely describe the aberration of the eye. With the recent advances in Wavefront Sensing technology, it is now feasible to accurately model the high-order aberrations present in each person's eye and thus obtain good models of various aberrations currently not correctable through conventional means (e.g., spectacles, contact lenses). Using these models, it would be possible to provide persons with currently uncorrectable aberrations a new alternative to enhance their interaction with computers.

The traditional optical correction of visual limitations uses physical means to modify the images of external objects just before they reach the eye. In contrast, the approach described here is based on modifying the image at its source, i.e., it suggests the application of image processing modifications on the image to be displayed on-screen before it is shown to the user, based on the knowledge of his/her wavefront aberration function. The aim of the pre-compensation proposed is to modify the intended display image in a way that is opposite to the effect of the wavefront aberration of the eye. Once this is achieved, the result is displayed to the viewer so that the effect of the wavefront aberration in the viewer's eye will "cancel" the pre-compensation resulting in the projection of an undistorted version of the intended image on the retina.

## 2. METHODOLOGY

### Imaging in the eye as a convolution process

In recent years, optical systems have begun to be analyzed as linear, shift-invariant systems described by their point spread function (PSF). This new conceptualization of optical systems has also been extended to the study of the human eye[2]. Therefore, the eye can be characterized by its PSF,  $T(x, y)$ , and the retinal image,  $R(x, y)$ , can be found by convolving (denoted by  $\otimes$ ) the input to the system, i.e., the image of the object to be seen,  $I(x, y)$ , with the PSF of the eye:

$$R(x, y) = I(x, y) \otimes T(x, y) \quad (1)$$

In a situation where a user views a computer screen, the real world image,  $I(x, y)$ , is stored as a digital image,  $DI(x, y)$ , which is then displayed to the user on a monitor/LCD. The retinal image, in this case, will be formed by convolution of the on-screen image and the PSF of the viewer's eye:

$$R(x, y) = DI(x, y) \otimes T(x, y) \quad (2)$$

However, in this special case, the on-screen image to be displayed to the user can be manipulated in advance. If the inverse PSF of the viewer's eye,  $T^{-1}(x, y)$ , could be defined, then an image,  $RD(x, y)$ , which is the result of convolving the intended digital image,  $DI(x, y)$ , with this inverse function could be shown to the viewer:

$$RD(x, y) = DI(x, y) \otimes T^{-1}(x, y) \quad (3)$$

Then, substituting the ordinary  $DI(x, y)$  with the pre-compensated  $RD(x, y)$ , in Eq. (2):

$$R(x, y) = \{DI(x, y) \otimes T^{-1}(x, y)\} \otimes T(x, y) = DI(x, y) \quad (4)$$

Eq. (4) suggests that the user would perceive in  $R(x, y)$  an undistorted version of the intended digital image,  $DI(x, y)$ . The image represented by the braces in Eq. (4) can also be considered to be the result of deconvolving the PSF,  $T(x, y)$ , from the intended image,  $DI(x, y)$ . This is the pre-compensated image to be displayed to the viewer. In practice, the deconvolution process may be performed more efficiently in the frequency domain, as discussed below. In any case, it is clear that, in order to obtain  $RD(x, y)$ , the PSF of the eye must be known or estimated.

#### Evaluation of the PSF of the human eye

The PSF of the human eye can be found indirectly through an associated optical performance measure, known as the wavefront aberration function,  $W(x, y)$ , for which practical measurement mechanisms are available. The wavefront aberration function represents the deviation of the light wavefront from a purely spherical pattern as it passes the pupil on its way to the retina [3]. In an unaberrated eye, the refracted light is organized in the form of a uniform spherical wavefront, converging to the paraxial focal point on the retina.

In the last decade "Wavefront Analyzers" based on the Hartmann-Shack Principle, have emerged and become commercially available for clinical use. These systems provide a practical means for the measurement of the wavefront aberration function in the human eye. In turn, the wavefront aberration function,  $W(x, y)$ , is the primary component of the pupil function,  $P(x, y)$ . The pupil function incorporates the complete information about the imaging properties of the optical system [4], and is defined as:

$$P(x, y) = A(x, y) e^{-j \cdot 2 \cdot \pi \cdot n \cdot W(x, y)} \quad (5)$$

where  $A(x, y)$  is the amplitude function describing the relative efficiency of light passing through the pupil (usually given a value of one), and  $n$  is the index of refraction [3].

Furthermore, the pupil function is linked through Fourier optics relationships in the eye to the optical transfer function,

OTF, which is "one of the most powerful descriptors of imaging performance for an optical system" [3]. The OTF is a complex function whose magnitude is the modulation transfer function (MTF) and whose phase is the phase transfer function (PTF) [3].

The OTF can be found by convolving the pupil function,  $P(x, y)$ , with its complex conjugate,  $P^*(-x, -y)$  [2], [3]:

$$O(f_x, f_y) = P(x, y) \otimes P^*(-x, -y) \quad (6)$$

which is equivalent of saying that the OTF is the autocorrelation of the pupil function. The PSF and the OTF are a Fourier transform pair [5]:

$$O(f_x, f_y) = F\{T(x, y)\} \quad (7)$$

The wavefront aberration function,  $W(x, y)$ , is usually represented by a Zernike polynomial expansion. These polynomials are two-dimensional functions that form a complete orthogonal basis set defined on the unit disc. They have been used in optical engineering for over 60 years, [6], [7]. Consequently, the Zernike polynomials have also been applied to the characterization of aberrations of the human eye [8], [9], [10]. Modern ophthalmic wavefront analyzers provide an approximation to the wavefront aberration function measured from the subject as a combination of Zernike polynomials. As indicated by Eqs. (5), (6), and (7), this characterization of the optics of the eye can be used to determine its PSF and OTF, thus enabling the implementation of the deconvolution concept expressed in Eqs. (3) and (4), as detailed below.

#### Inverse Filtering as a means of deconvolution

In the field of image processing, inverse filtering is frequently used to achieve image restoration, i.e., to attempt to recover an image  $U(x, y)$  from a degraded image  $G(x, y)$ , assuming a known degradation function,  $H(x, y)$ . As stated above, the input and output of any linear system are related through the convolution operator. That is,

$$G(x, y) = U(x, y) \otimes H(x, y) \quad (8)$$

According to the Fourier principles of convolution,  $U(x, y)$  can be obtained as follows:

$$U(x, y) = F^{-1} \left\{ \frac{F\{G(x, y)\}}{F\{H(x, y)\}} \right\} \quad (9)$$

where  $F\{\cdot\}$  and  $F^{-1}\{\cdot\}$  denote the Fourier transform and the inverse Fourier transform, respectively.

When pre-compensating a digital image to be shown to the viewer, the objective is to deconvolve the PSF of the viewer's eye,  $T(x, y)$ , from the intended digital image,  $DI(x, y)$ , in order to derive the pre-compensated display image to show on-screen,  $RD(x, y)$ . Making the corresponding substitutions in Eq. (9), the calculation of  $RD(x, y)$  is mathematically accomplished as:

$$RD(x, y) = F^{-1} \left\{ \frac{F\{DI(x, y)\}}{F\{T(x, y)\}} \right\} \quad (10)$$

Eq. (10) represents the process commonly known as inverse filtering in frequency, and is equivalent to two-dimensional deconvolution in the spatial domain. It should be noted that, according to Eq. (7), the denominator within the braces of Eq. (10) is the OTF of the viewer's eye.

This implementation of inverse filtering, however, has several limitations, especially for values of the PSF or its frequency counterpart, the OTF, which are close to zero. A common approach to circumvent this problem is the use of Minimum Mean Square Error filtering [11]. In the context of the problem at hand, this approach obtains the pre-compensated image as:

$$RD(fx, fy) = \left[ \frac{1}{T(fx, fy)} \frac{|T(fx, fy)|^2}{|T(fx, fy)|^2 + K} \right] DI(fx, fy) \quad (11)$$

where  $RD(fx, fy)$ ,  $T(fx, fy)$ , and  $DI(fx, fy)$  are the Fourier transforms of  $RD(x, y)$ ,  $T(x, y)$ , and  $DI(x, y)$ , respectively. In addition to the limitation of values in the pre-compensated image, the approach indicated in Eq. (11) helps reduce the impact of modeling or measurement noise inherent to the definition of the eye's PSF. The  $K$  factor in Eq. (11) should be proportional to the magnitude of the estimation noise in the PSF approximation.

### 3. RESULTS AND DISCUSSION

#### Testing

Quantification of the results was done with the participation of human subjects. In order to proceed with the testing of the pre-compensation method proposed, human subjects having a satisfactory standard visual acuity of 20/20 [12], either corrected or natural, were recruited. Then, a refractive error, specifically a defocus, was artificially introduced in their field of view by means of a pre-selected lens. A similar procedure was used by Sonksen to test visual function [13].

In order to provide a well-known and standardized method of reporting visual performance, a standard Eye Test Chart was used. The characters of a Bailey-Lovie visual acuity chart with 'Sloan' letters (Figure 1) were reproduced as properly sized digital images for the tests.

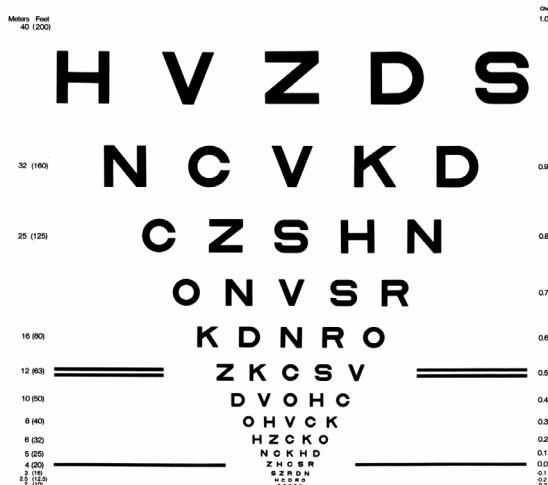


Figure 1- Bailey-Lovie Eye Test Chart

#### Simulated Experiment for -6.00 Diopter Sphere Lens

The PSF of a -6.0 diopter (D) lens was obtained by means of Eq. (11) using the image of a point source of light in dark background, which replaces  $T(x, y)$ , and the image of the same scene, viewed through the lens replacing  $DI(x, y)$ . This PSF estimation, as well as the generation of the pre-compensated image, was accomplished using MATLAB®. Figure 2 shows the analytical PSF obtained, using the wavefront aberration function corresponding to a -6.0 D lens, scaled and resized. A comparison of the two PSF, both analytical and empirical is necessary to ensure the proper pre-compensation. Once the analytical PSF is verified to be similar to the empirical PSF, the analytical is used to apply the pre-compensation. The empirical PSF contains a great deal of noise which hinders the deconvolution process, making even more ill-posed.

Additionally, the analytical PSF has been cropped and padded to match the image size of a line from a standard eye test chart, shown in Figure 3. This is necessary due to the fact that both the image and the PSF need to be of the same size in order to implement the minimum mean square error deconvolution described by Eq. (11). Another key factor to this process is that the eye test chart lines, when displayed on-screen, must be equivalent in size to an actual eye test chart. This is important because it ensures that the test can be properly administered.

Figure 4 shows a simulation of the upper line of the eye test chart, as seen by the experimental subjects through the -6.0 D lens. This simulation is obtained by convolution of the analytical PSF (Figure 2) with the image in Figure 3.

Figure 5 shows the result of applying the pre-compensation process to the image in Figure 3. This is the image that compensates for the aberration introduced by the -6.0 D lens. This image was produced using Eq. (11) with a  $K$  value of 0.0005.

Figure 6 shows a simulation of the result of the pre-compensation process obtained by convolving Figure 5 with the PSF of the lens (Figure 2).

#### Human Subject Testing Results

The results of testing with human subjects are shown in Figure 7. This figure shows the visual acuity in logMAR units for fourteen subjects. Each of their eyes was studied independently resulting in twenty-eight visual acuity scores. With respect to Figure 7, the bottom trace indicates the visual acuities obtained for the eye test without any blur or pre-compensation. The top trace (dashed line) indicates the values through the blur, and the center trace represents the values obtained from the pre-compensated eye test. A smaller value of visual acuity indicates the ability of the subject to correctly read further down the chart in a standard eye test. For reference, a logMAR value of 1.4 at a viewing distance of two meters represents a misreading of all of the largest letters on the eye test chart.

As can be seen from Figure 7, the pre-compensation partially restored the vision of the subjects, allowing them to read further down the eye test chart.



Figure 2- Analytical PSF of the -6.0 D lens used in the tests.

H V Z D S

Figure 3- Digital Representation of one line from a standard eye test chart



Figure 4- Simulated blur caused by the PSF in Figure 1



Figure 5- Resulting pre-compensated image



Figure 6- Simulated image of what the subject would see when viewing Figure 3 through the -6.0 diopter lens.

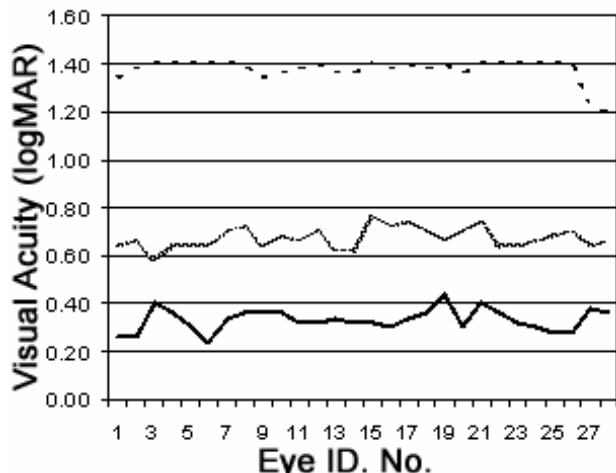


Figure 7- Results with human subjects

#### 4. CONCLUSION

This paper has proposed a framework for pre-compensation of digital images before they are displayed to low-vision users on a computer screen in order to compensate for their visual limitations. The results shown in Figure 7 demonstrate that this is indeed possible, and that the method presented in this paper, when applied to digital on-screen images, partially restores the vision of subjects with an artificial, second-order aberration

introduced into their field of view. Although this example pre-compensates for a low-order aberration, it should be noted that this framework also contemplates the correction of higher-order optical aberrations that are not addressed by current visual correction methods.

#### 5. ACKNOWLEDGMENT

This work was sponsored by NSF grants IIS-0308155 and HRD-0317692. Mr. Miguel Alonso Jr. is the recipient of a Graduate Research Fellowship from the National Science Foundation.

#### 5. REFERENCES

- [1] Perry, S.W., H.S. Wong, and L. Guang, **Adaptive Image Processing: A Computational Intelligence Perspective**, CRC Press, New York, 2002.
- [2] Thibos, L.N., "Formation and Sampling of the Retinal Image", Chapter 1 in **Seeing, A volume in the Handbook of Perception and Cognition Series**, Karen K. De Valois, ed. Academic Press, California, 2000.
- [3] Salmon, T.O., "Corneal Contribution to the Wavefront Aberration of the Eye", **Doctoral Dissertation, School of Optometry**, Indiana University, 1999.
- [4] Williams, C.S., O.A Becklund, **Introduction to the Optical Transfer Function**, John Wiley and Sons, Inc, New York, 1989.
- [5] Bracewell, R.N, **Two-Dimensional Imaging**, Prentice-Hall Signal Processing, New Jersey, 1995.
- [6] Born, M., and E. Wolf, **Principles of Optics**, 6th Edition, Pergamon Press, Oxford.
- [7] Malacara, D., **Optical Shop Testing**, Jon Wiley and Sons, Inc, New York.
- [8] Webb, R., **Zernike Polynomial description of ophthalmic surfaces**, OSA Technical Digest Series, Ophthalmic and Visual Optics, 1992.
- [9] Liang, J., Grimm, B., Goelz, S. & Bille, J. F., **Objective measurement of wave aberrations of the human eye with the use of a Hartmann-Shack wave-front sensor**, J Opt Soc Am A, 1994.
- [10] Liang, J. & Williams, D. R., **Effect of higher order aberrations on image quality in the human eye**, OSA Technical Digest Series (Vision Science and Its Applications), 1995.
- [11] Gonzales, R.C., and R.E. Wood, **Digital Image Processing**, Second Edition, Prentice Hall, New Jersey, 2002.
- [12] Bennet, A.G., and R.B Rabbets, **Clinical Visual Optics**
- [13] Sonksen, P. M., and A. J. Ma, Second Edition, Butterworths, London, 1989.crae, "Vision for coloured pictures at different acuities: the Sonksen Picture Guide to Visual Function", **Developmental Medicine Child Neurology**, 29: pp. 337-347, 1987.